



2.0 - 6.8 MHz
Convex C3-E



4.0 - 15.0 MHz
Linear L7-E



7.0 - 18.0 MHz(With FHI)
Linear L12-E



4.0 - 15.0 MHz
Linear L7W-E



4.0 - 12.0 MHz
Transvaginal V6-E



4.0 - 15.0 MHz
Transvaginal V7-E



4.0 - 15.0 MHz
Trans-Rectal
L7R-E



2.0 - 6.8 MHz
Micro-Convex MC3-E




4.0 - 12.0 MHz
Micro-Convex MC6-E



HIP Graf



Gallbladder stone, B Mode

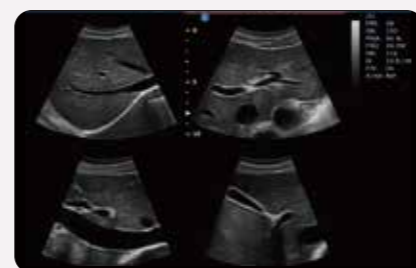


Abdomen, 4B Mode



Pancreas, B/BC Mode




Umbilical cord, C Mode

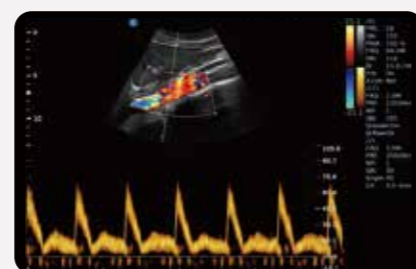


Aorta Artery, PW Mode



CCA, ICA, ECA, B Mode

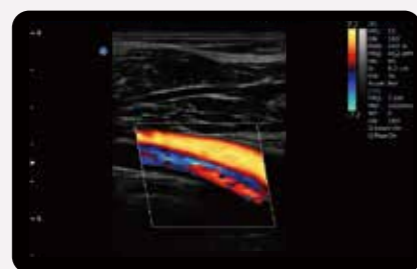

Popliteal Artery and Vein

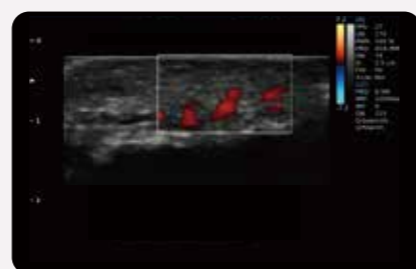

Fingertip Vessle, C Mode

EBit 30



CHISON Medical Technologies Co., Ltd.

Sales & Service Contact Address:
No.9, Xinhuihuan Road, Xinwu District, Wuxi, Jiangsu, China 214028
TEL : 0086-510-85310593 / 85310937 FAX : 0086-510-85310726 EMAIL : export@chison.com.cn

We reserve the right to make changes to this catalogue without prior notice
Please contact our local dealer for the latest information.

EBit 30-20181207

Ergonomic Design


I need a portable, light-weight ultrasound which is easy to go, easy to diagnose, easy to operate with sufficient measurement packages.

- Independent angle 15" LED (0° - 30° tilted)
- Lightweight (7.5Kg / 16.5lbs)
- Dual transducer ports (Built-in)
- Probe holders
- Removable battery , 120 minutes in active mode
- Theft-proof lock
- Dedicated adapter Space
- Printer socket
- Accessory box
- Trolley height adjustable (Three levels available)




FHI

- FHI is an innovative harmonic imaging technology that uses multiple transmission and receiving methods based on the patients' size and weight. This allows the EBit to maintain image resolution when imaging larger patients.
- Traditional Tissue Harmonics and Phased Harmonics compromise image quality and resolution when penetration is increased.
- Chison's FHI technology greatly improves diagnostic abilities and clinical confidence in larger, difficult-to-image patients.

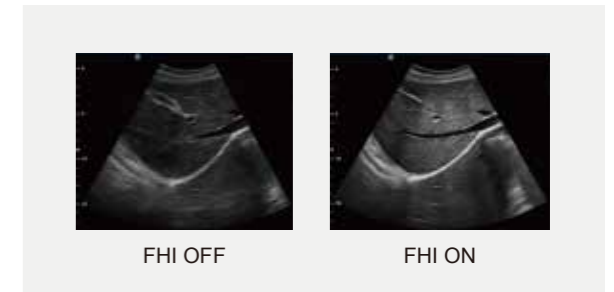


Q-image

- These innovative algorithms have strengthened the image enhancement results significantly.
- Advanced chipset is used to ensure fast frame rate.

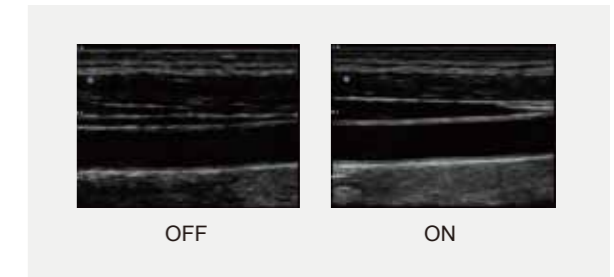


Q-beam

- Compared to the traditional dual-beam former on most ultrasound machines, the EBit50 uses quad-beam technology for ultrasound signal receiving.
- Doubles the volume of signals received from traditional methods, increasing image resolution and generating more accurate images.
- Produces higher frame rates, ensuring better diagnostic confidence and efficiency, especially for moving organs.

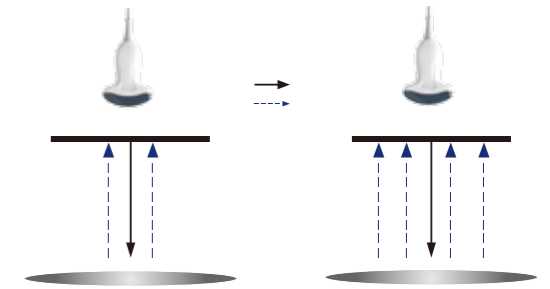

Auto IMT

Automatically traces the intima, and measures the thickness of the intima. This allows you to measure the intima faster, more easily and more accurately.

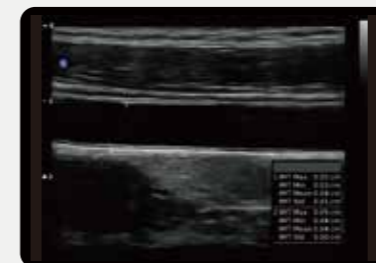

Elastography

Elastography displays tissue stiffness in real time to provide doctors with additional diagnostic information when scanning organs like liver and breast.

